


User's Guide

Product Code: arFX001



Warning

- All persons using this product must receive user training.
- Do not lean back too far on the device.
- The product does not have functions for preventing falls.
- The user must keep balance on his/her own.
- Please only use the product to support your posture during standing tasks.
- The product is not intended for uses who have difficulty in walking normally due to disability or other reasons.

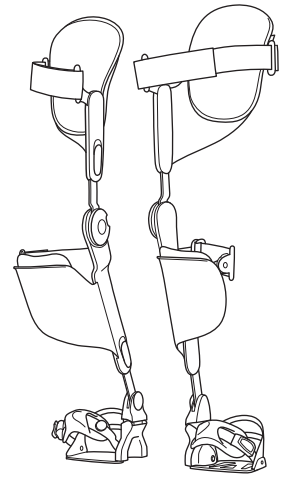

How to Use This Product Safely in the Long Term

Thank you for purchasing our product. Please read this guide carefully and use the product correctly.



Safety Precautions

Please fully observe the following precautions to prevent injury or harm to you or others, as well as to ensure safe use of the product.


- The amount of time it takes for users to get used to wearing the device varies from person to person. Follow your trainer's instructions and gradually get used to wearing the unit.
- If you need to use the device before receiving training, follow this manual and learn to use the device correctly from a person who has been trained.
- Be careful not to pinch your fingers with the frame during installation.
- Please change your posture as appropriate during use when wearing the device on an ongoing basis.
- If you use the device while staying in the same posture for a long period of time, blood clot may occur from the strain being put on the leg.
- Do not use the product with bare feet, high-heeled footwear, or ill-fitting work pants.
- Do not use the device in bumpy, unlevel areas with obstacles, as this is a trip and fall hazard.
- Do not hold heavy objects while wearing the product. The product does not have functions for distributing the load from heavy objects.



Handling Precautions

- The product is for indoor use. Do not use it outdoors.
- When storing this product, please put it indoors on a flat surface.
- Please store the device away from high temperature, humidity, and direct sunlight.
- Inspect the product periodically to ensure safe use.
- When carrying the product, please be careful not to drop on your feet.
- The product is covered by a 3-year warranty. However, the warranty does not cover any damage resulting from violations of safety/handling precautions and unauthorized modifications. Moreover, after the warranty period expires, you become liable for all repair fees.
- Do not hold heavy objects while wearing the product. The product does not have functions for distributing the load from heavy objects.
- Make sure there are no young children nearby when using.
- Do not ride a motorcycle or bicycle while wearing the product.
- archelis will not be liable for any damages or injury arising directly or indirectly from the use of the product.
- If a malfunction occurs in the product, contact your distributor.
- Please note that the product design, specifications, appearance, and price are subject to change without prior notice for product improvement.
- archelis will not be liable for any physical injuries, property damage, or other types of damage caused by improper use of the product.

Names of Parts

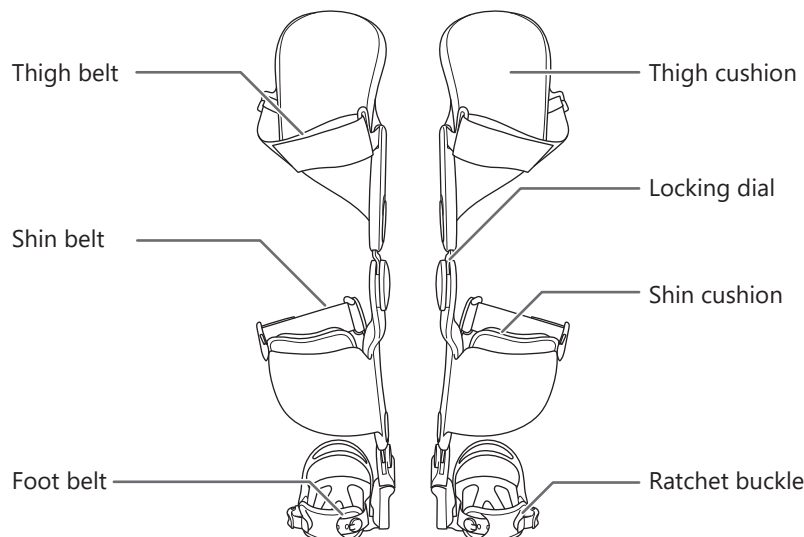

Before using


Please check the following before use:

- Check that the device locks properly.
- Check that each mode is functioning properly.
- Check that there are no cracks and loose screws/pins on any of the parts.
- Check that there is no deformation in any of the parts.
- Adjust it to your own body size. Improper sizing may reduce the effectiveness of the product.


Length Adjustment (Shin and Thigh Parts)

Before putting on the device, you need to adjust the positions of the shin and thigh parts so that the device can fit your height and body shape.


The following procedure describes how to adjust the shin parts. Please also use this procedure to adjust the thigh parts.

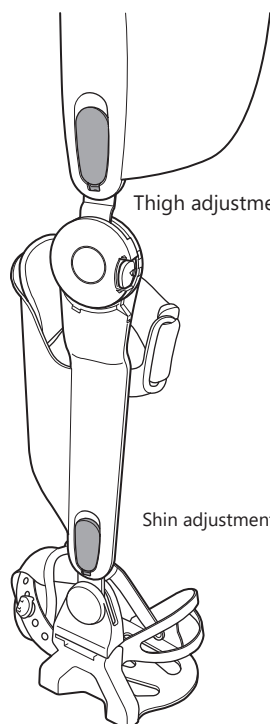


01 Pull open the cover.




02 Take out the set pin.




03 Adjust the part to the position with the scale marks that match your height, as shown in the table below.



04 Reinsert the set pin that was taken out in the step 2.



05 Close the cover.



Scale Positions by Height Range

S size

Scale		Height range (ft/in)
Shin part	Thigh part	
•	•	4' 9" - 4' 11"
••	••	4' 12" - 5' 2"
•••	•••	5' 2" - 5' 5"

M size

Scale		Height range (ft/in)
Shin part	Thigh part	
•	•	5' 3" - 5' 5"
••	••	5' 5" - 5' 8"
•••	•••	5' 8" - 5' 10"
••••	••••	5' 11" - 6' 1"

L size

Scale		Height range (ft/in)
Shin part	Thigh part	
•	•	5' 7" - 5' 9"
••	••	5' 10" - 5' 12"
•••	•••	6' - 6' 3"
••••	••••	6' 3" - 6' 5"



Adjustment of Parts and Accessories

Please adjust the following parts and accessories to fit the user.

- Please use the length adjustment (shin and thigh parts) table for reference.

Adjust the parts so that the device fits the user's height and body shape.

Example: If the user's height is 170 cm, adjust the shin and thigh parts to the positions where the "●●" and "●●●" scale marks are shown respectively.

- There are cushions in 2 locations (front of the shin part, back of the thigh part) for each leg.


Adjust the position of these so that the device fits the user's height and body shape.




How to Adjust the Foot Belt Strap Length (Ratchet Buckle Type)

Before putting on the device, you need to adjust the strap length so that the strap can fit your shoe.


01 Push the knob upward.

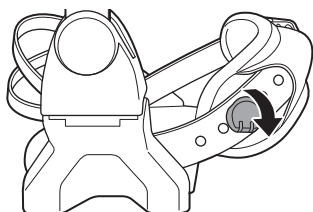


02 Turn the knob counterclockwise, then remove it.

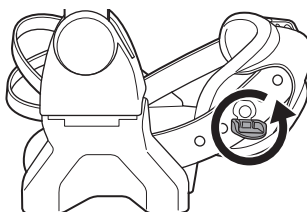


03 Adjust the strap length to suit your shoe size.

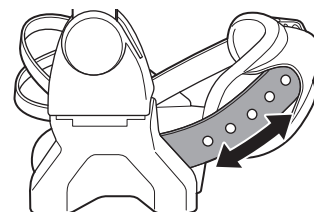

04 Turn the knob clockwise until tight.

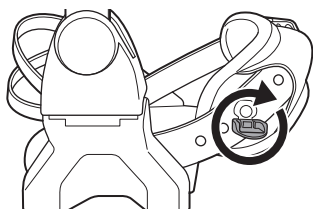

05 Push the knob back down.

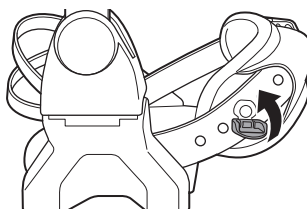




Putting on the Device

Please put the device on starting with the foot, shin, then thigh parts in that order.
Be careful not to pinch your fingers with the frame during installation.

01 Foot


02 Shin

03 Thigh

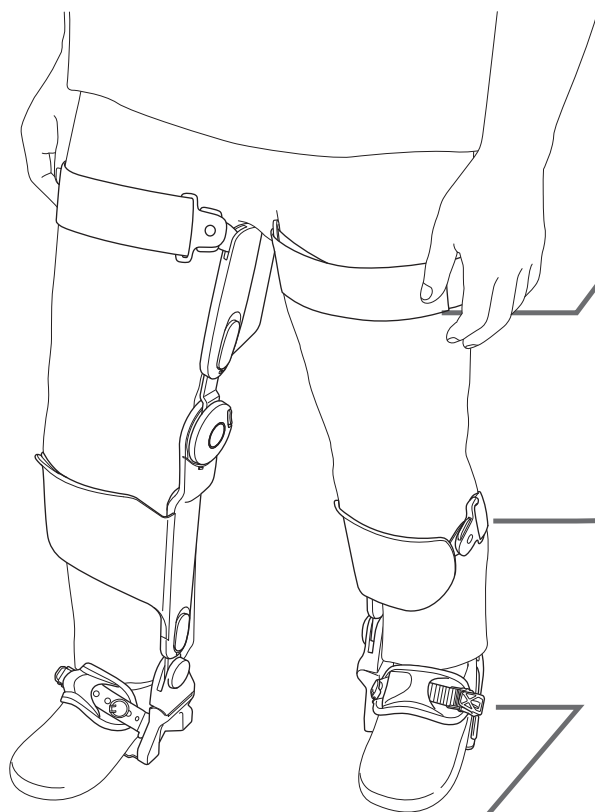


03 Thigh

Fix to your thigh with the thigh belt.



02 Shin

Fix to your shin with the shin belt.

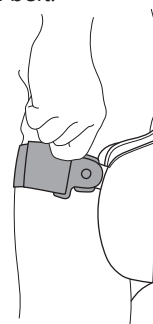

01 Foot




Adjust your heel to the foot part of the device.



Insert the ladder strap into the ratchet buckle.




Pull the ratchet buckle handle downwards to fix the ladder strap.

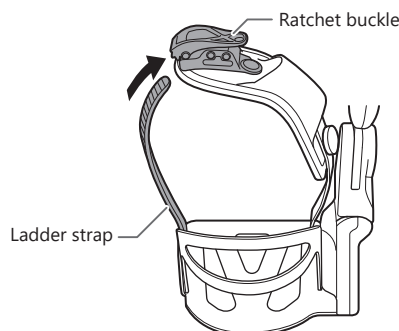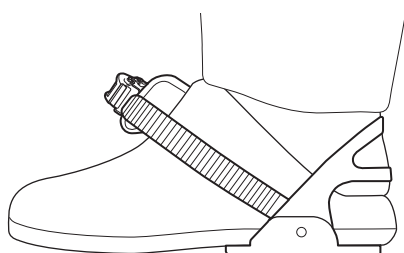

How to Unfasten From the Foot

Push the ratchet buckle handle upwards to release the ladder strap.




How to use the locking dials


The locking dial can be turned to switch modes only when the user's weight is not being put on the product. After changing modes with wearing gloves, earplugs, etc., make sure the product is locked before applying your body weight.

The following procedure describes how to switch from archelis mode to free mode.

01 Turn the dial slightly while holding down the orange-colored button, and then release the button.

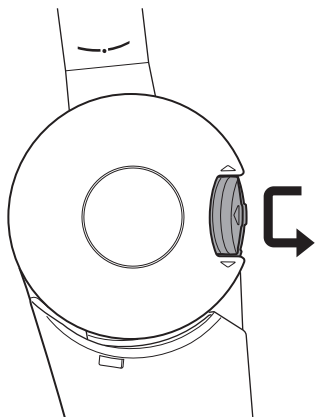



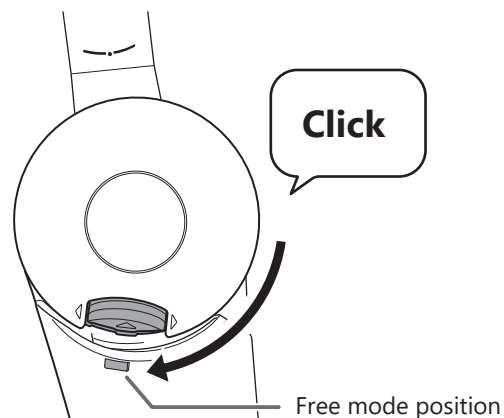



02 When the button is released, turn the dial to a mode position, which sounds with a click.




About Modes

The product provides 3 modes to suit different levels of ease when walking and standing position retention. You can switch modes using the locking dials.

	Free mode	archelis mode	Standing mode
Ease of walking	◎	○	△
Standing position retention	Does not retain standing position	Retains half crouching position	Retains upright standing position
Image of posture			
Position of the locking dial for each mode (Figure indicates the position of the dial on the right leg.)			

⚠ Do not sit down when in free mode. Doing so may damage the device.

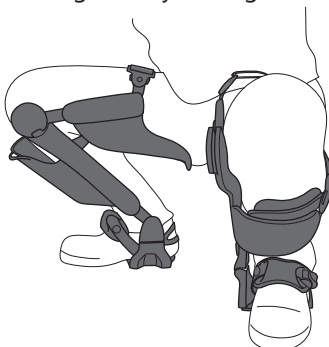




How to replace the foot parts


The foot parts are replaceable between ratchet buckle type and stick type. Select the appropriate type according to the operating environment and work process. When using the stick type, an ankle belt must be attached.

This section describes the procedure for replacing the ratchet buckle with the stick type.


01 Pull open the cover.




02 Take out the set pin.




03 Remove the ratchet buckle type foot parts from archelis.

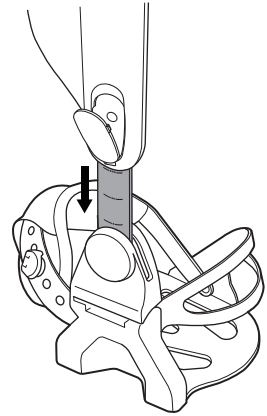


04 Insert the stick type foot part.

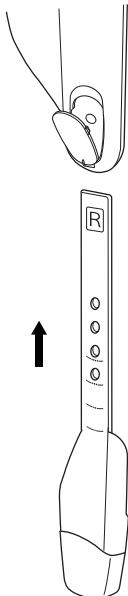

05 Reinsert the set pin that was taken out in the step 2.

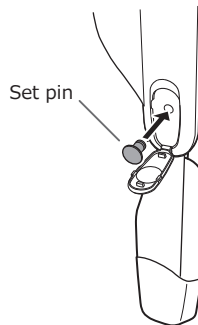

06 Close the cover.



Maintenance

Regular Maintenance

<Cleaning the resin and metal parts>

- Please always clean the resin and metal parts before using.
- If there is heavy soiling in the resin and metal parts, wipe clean using a cloth that has been dampened with water or neutral detergents and wrung out. After that, wipe again using another soft and dry cloth.
- Do not let liquids enter into the moving parts of the device.
- If the lifter unit and foot rubber are worn out, they need to be replaced.

<Cleaning cushion parts>

- Pat the dust off the parts with fabric and then vacuum any remaining dust with a vacuum cleaner.
- Put cushion parts into a laundry net to wash.
- If there is visible soiling, replace with a new cushion (sold separately).

<Cleaning in a Clinical Site>

- Wipe the device thoroughly every time you use it.
Be sure to use an appropriate amount of liquid detergent, such as a neutral detergent, ethanol for disinfection, or hydrogen peroxide, when cleaning.
- Do not let liquids enter into the moving parts of the device.
- Make sure you have completely removed any blood stains, dead skin, or salt-edged patches from the surface of the device.
- After wiping the product clean, wipe it dry again with distilled or sterile water.
- Do not use ultrasonic cleaners or jet-type instrument cleaners.

Malfunctions

- If you find any abnormalities with the product, contact your distributor.

Disposal Methods

- Separate each part and dispose of it as industrial waste. If disposal is difficult, please contact the distributor.

<Distributor>

<Manufacturer>

Troubleshooting

Use the following information for troubleshooting.

Symptoms & Condition	Remedy
Locking dial cannot be turned	Turn the dial without putting any weight on the device.
Device fell over	Switch to free mode and then stand up.
Device cannot be locked normally	Stop using and contact your distributor.
Device makes abnormal noises	Stop using and contact your distributor.

Product Specifications

Product Name	archelisFX		
Product Code	arFX001-S	arFX001-M	arFX001-L
Wearable Height	4' 9" - 5' 5"	5' 3" - 6' 1"	5' 7" - 6' 5"
Max. Load Weight	Up to 143 lb	Up to 198 lb	Up to 254 lb
Dimensions(one leg)	6.9×11.0×28.1 inch	6.9×11.0×30.9 inch	6.9×11.0×32.4 inch
Weight (one leg)	4.4 lb	4.6 lb	5.5 lb
Number of adjustable positions	3 positions (free mode included)		